

Certificate number: o60247005i246288-B-1



# Calibration Certificate

Customer  
UPSTATE MEDICAL PHYSICS  
BLOSSOM DR 1290  
14564 VICTOR  
US

Laboratory  
Unfors RaySafe Inc.  
2 Science Road  
Glenwood, IL 60425-1586  
USA  
+1-833-296-9240  
customerservice.us@raysafe.com

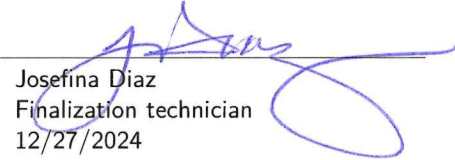
## CUSTOMER INSTRUMENT

Product X2 R/F  
Serial number 246288  
Manufacturer RaySafe

## CALIBRATION INFORMATION

As found 12/14/2024  
As left 12/17/2024  
Adjustment done Yes  
Tested by Christina Arroyo

Approved by

  
Josefina Diaz  
Finalization technician

Certificate date 12/27/2024



# Calibration Certificate



Customer  
UPSTATE MEDICAL PHYSICS  
BLOSSOM DR 1290  
14564 VICTOR  
US

Laboratory  
Unfors RaySafe Inc.  
2 Science Road  
Glenwood, IL 60425-1586  
USA  
+1-833-296-9240  
customerservice.us@raysafe.com

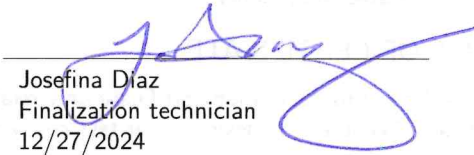
## CUSTOMER INSTRUMENT

Product X2 R/F  
Serial number 246288  
Manufacturer RaySafe

## CALIBRATION INFORMATION

As found 12/14/2024  
As left 12/17/2024  
Adjustment done Yes  
Tested by Christina Arroyo

Approved by

  
Josefina Diaz  
Finalization technician

Certificate date 12/27/2024

## CALIBRATION RESULT

AS FOUND: All measured and tested values of this certificate were found to be in conformance with the specification.

AS LEFT: All measured and tested values of this certificate were found to be in conformance with the specification.

Relevant instrument specifications

Air kerma: 5 %, Air kerma rate: 5 %  
Time: 0.5 %, Voltage: 2 %

This laboratory is accredited according to ISO/IEC 17025:2017 by the American Association for Laboratory Accreditation (A2LA) and the results shown in this certificate have been determined within the scope of accreditation unless stated otherwise in this certificate.



Certificate number: o60246909i246204-B-1



# Calibration Certificate

Customer  
UPSTATE MEDICAL PHYSICS  
BLOSSOM DR 1290  
14564 VICTOR  
US

Laboratory  
Unfors RaySafe Inc.  
2 Science Road  
Glenwood, IL 60425-1586  
USA  
+1-833-296-9240  
customerservice.us@raysafe.com

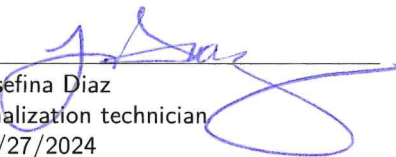
## CUSTOMER INSTRUMENT

Product X2 MAM  
Serial number 246204  
Manufacturer RaySafe

## CALIBRATION INFORMATION

As found 12/12/2024  
As left 12/17/2024  
Adjustment done Yes  
Tested by Armad Bryant  
Maria Isabel Magana Guerrero  
Nate Barnes  
Rosio Ramos  
Tommy Cox

Approved by

  
Josefina Diaz  
Finalization technician

Certificate date

12/27/2024



# Calibration Certificate



Customer  
UPSTATE MEDICAL PHYSICS  
BLOSSOM DR 1290  
14564 VICTOR  
US

Laboratory  
Unfors RaySafe Inc.  
2 Science Road  
Glenwood, IL 60425-1586  
USA  
+1-833-296-9240  
customerservice.us@raysafe.com

## CUSTOMER INSTRUMENT

Product X2 MAM  
Serial number 246204  
Manufacturer RaySafe

## CALIBRATION INFORMATION

As found 12/12/2024  
As left 12/17/2024  
Adjustment done Yes  
Tested by Armad Bryant  
Maria Isabel Magana Guerrero  
Nate Barnes  
Rosio Ramos  
Tommy Cox

Approved by

Josefina Diaz  
Finalization technician

Certificate date

12/27/2024

## CALIBRATION RESULT

**AS FOUND:** One or more measured and tested values of this certificate are within the specifications by a margin less than the expanded measurement uncertainty. Therefore, it is not possible to state conformance with specifications for those measurements.

**AS LEFT:** All measured and tested values of this certificate were found to be in conformance with the specification.

Relevant instrument specifications

Air Kerma: 5 %

Voltage: 2 % or 0.5 kV (without paddle), 2 % or 0.7 kV (with paddle)

This laboratory is accredited according to ISO/IEC 17025:2017 by the American Association for Laboratory Accreditation (A2LA) and the results shown in this certificate have been determined within the scope of accreditation unless stated otherwise in this certificate.



# Calibration Certificate



Customer  
UPSTATE MEDICAL PHYSICS  
BLOSSOM DR 1290  
14564 VICTOR  
US

Laboratory  
Unfors RaySafe Inc.  
2 Science Road  
Glenwood, IL 60425-1586  
USA  
+1-833-296-9240  
customerservice.us@raysafe.com

## CUSTOMER INSTRUMENT

Product X2 Survey  
Serial number 230028  
Manufacturer RaySafe

## CALIBRATION INFORMATION

As found 12/17/2024  
As left 12/17/2024  
Adjustment done Yes  
Tested by Armad Bryant

Approved by

Josefina Diaz  
Finalization technician

Certificate date 12/27/2024

## CALIBRATION RESULT

AS FOUND: All measured and tested values of this certificate were found to be in conformance with the specification.

AS LEFT: All measured and tested values of this certificate were found to be in conformance with the specification.

Relevant instrument specifications

Air kerma: 5 % (RQA), 10 % (N-series)

This laboratory is accredited according to ISO/IEC 17025:2017 by the American Association for Laboratory Accreditation (A2LA) and the results shown in this certificate have been determined within the scope of accreditation unless stated otherwise in this certificate.



# Calibration Certificate

Customer  
UPSTATE MEDICAL PHYSICS  
BLOSSOM DR 1290  
14564 VICTOR  
US

Laboratory  
Unfors RaySafe Inc.  
2 Science Road  
Glenwood, IL 60425-1586  
USA  
+1-833-296-9240  
customerservice.us@raysafe.com

## CUSTOMER INSTRUMENT

Product X2 Light  
Serial number 232790  
Manufacturer RaySafe

## CALIBRATION INFORMATION

As found 12/20/2024  
As left 12/20/2024  
Adjustment done Yes  
Tested by Amber Ramos

Approved by

  
Josefina Díaz  
Finalization technician

Certificate date 12/27/2024

## CALIBRATION RESULT

AS FOUND: One or more measured and tested values of this certificate are within the specifications by a margin less than the expanded measurement uncertainty. Therefore, it is not possible to state conformance with specifications for those measurements.

AS LEFT: All measured and tested values of this certificate were found to be in conformance with the specification.

Relevant instrument specifications

Illuminance: 3 %  
Luminance: 3 %



# Calibration Certificate



Customer  
UPSTATE MEDICAL PHYSICS  
BLOSSOM DR 1290  
14564 VICTOR  
US

Laboratory  
Unfors RaySafe Inc.  
2 Science Road  
Glenwood, IL 60425-1586  
USA  
+1-833-296-9240  
customerservice.us@raysafe.com

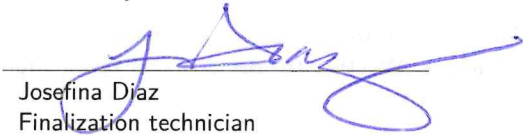
## CUSTOMER INSTRUMENT

Product X2 CT  
Serial number 224343  
Manufacturer RaySafe

## CALIBRATION INFORMATION

As found 12/16/2024  
As left 12/16/2024  
Adjustment done Yes  
Tested by Armad Bryant

Approved by

  
Josefina Djaz  
Finalization technician

Certificate date 12/27/2024

## CALIBRATION RESULT

AS FOUND: All measured and tested values of this certificate were found to be in conformance with the specification.

AS LEFT: All measured and tested values of this certificate were found to be in conformance with the specification.

Relevant instrument specifications

Air kerma: 5 %

This laboratory is accredited according to ISO/IEC 17025:2017 by the American Association for Laboratory Accreditation (A2LA) and the results shown in this certificate have been determined within the scope of accreditation unless stated otherwise in this certificate.

