

Certificate number: o60247002i311361-A-1



Calibration Certificate



Customer
UPSTATE MEDICAL PHYSICS
BLOSSOM DR 1290
14564 VICTOR
US

Laboratory
Unfors RaySafe Inc.
2 Science Road
Glenwood, IL 60425-1586
USA
+1-833-296-9240
customerservice.us@raysafe.com

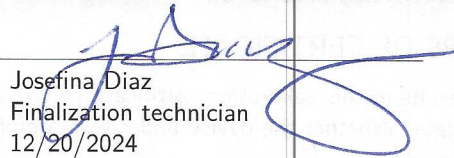
CUSTOMER INSTRUMENT

Product X2 R/F
Serial number 311361
Manufacturer RaySafe

CALIBRATION INFORMATION

As found 12/14/2024
As left 12/17/2024
Adjustment done Yes
Tested by Christina Arroyo

Approved by


Josefina Diaz
Finalization technician

Certificate date 12/20/2024

CALIBRATION RESULT

AS FOUND: All measured and tested values of this certificate were found to be in conformance with the specification.

AS LEFT: All measured and tested values of this certificate were found to be in conformance with the specification.

Relevant instrument specifications

Air kerma: 5 %, Air kerma rate: 5 %
Time: 0.5 %, Voltage: 2 %

This laboratory is accredited according to ISO/IEC 17025:2017 by the American Association for Laboratory Accreditation (A2LA) and the results shown in this certificate have been determined within the scope of accreditation unless stated otherwise in this certificate.



Certificate number: o60247002i311361-B-1



Calibration Certificate

Customer
UPSTATE MEDICAL PHYSICS
BLOSSOM DR 1290
14564 VICTOR
US

Laboratory
Unfors RaySafe Inc.
2 Science Road
Glenwood, IL 60425-1586
USA
+1-833-296-9240
customerservice.us@raysafe.com

CUSTOMER INSTRUMENT

Product X2 R/F
Serial number 311361
Manufacturer RaySafe

CALIBRATION INFORMATION

As found 12/14/2024
As left 12/17/2024
Adjustment done Yes
Tested by Christina Arroyo

Approved by


Josefina Djaz
Finalization technician

Certificate date

12/20/2024



Certificate number: o60246888i311863-B-1



Calibration Certificate

Customer
UPSTATE MEDICAL PHYSICS
BLOSSOM DR 1290
14564 VICTOR
US

Laboratory
Unfors RaySafe Inc.
2 Science Road
Glenwood, IL 60425-1586
USA
+1-833-296-9240
customerservice.us@raysafe.com

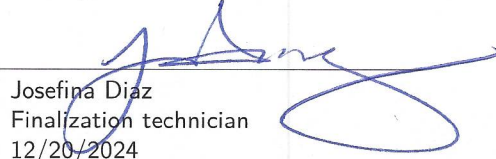
CUSTOMER INSTRUMENT

Product X2 MAM
Serial number 311863
Manufacturer RaySafe

CALIBRATION INFORMATION

As found 12/12/2024
As left 12/17/2024
Adjustment done Yes
Tested by Armad Bryant
Maria Isabel Magana Guerrero
Rosio Ramos
Tommy Cox

Approved by


Josefina Diaz
Finalization technician

Certificate date

12/20/2024



Certificate number: o60246888i311863-A-1



Calibration Certificate



Customer
UPSTATE MEDICAL PHYSICS
BLOSSOM DR 1290
14564 VICTOR
US

Laboratory
Unfors RaySafe Inc.
2 Science Road
Glenwood, IL 60425-1586
USA
+1-833-296-9240
customerservice.us@raysafe.com

CUSTOMER INSTRUMENT

Product X2 MAM
Serial number 311863
Manufacturer RaySafe

CALIBRATION INFORMATION

As found 12/12/2024
As left 12/17/2024
Adjustment done Yes
Tested by Armad Bryant
Maria Isabel Magana Guerrero
Rosio Ramos
Tommy Cox

Approved by

Josefina Diaz
Finalization technician

Certificate date

12/20/2024

CALIBRATION RESULT

AS FOUND: One or more measured and tested values of this certificate are within the specifications by a margin less than the expanded measurement uncertainty. Therefore, it is not possible to state conformance with specifications for those measurements.

AS LEFT: All measured and tested values of this certificate were found to be in conformance with the specification.

Relevant instrument specifications

Air Kerma: 5 %

Voltage: 2 % or 0.5 kV (without paddle), 2 % or 0.7 kV (with paddle)

This laboratory is accredited according to ISO/IEC 17025:2017 by the American Association for Laboratory Accreditation (A2LA) and the results shown in this certificate have been determined within the scope of accreditation unless stated otherwise in this certificate.



Calibration Certificate



Customer
UPSTATE MEDICAL PHYSICS
BLOSSOM DR 1290
14564 VICTOR
US

Laboratory
Unfors RaySafe Inc.
2 Science Road
Glenwood, IL 60425-1586
USA
+1-833-296-9240
customerservice.us@raysafe.com

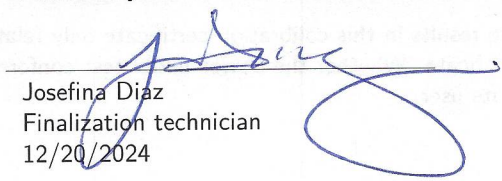
CUSTOMER INSTRUMENT

Product X2 Survey
Serial number 282096
Manufacturer RaySafe

CALIBRATION INFORMATION

As found 12/9/2024
As left 12/9/2024
Adjustment done Yes
Tested by Armad Bryant

Approved by


Josefina Diaz
Finalization technician

Certificate date 12/20/2024

CALIBRATION RESULT

AS FOUND: All measured and tested values of this certificate were found to be in conformance with the specification.

AS LEFT: All measured and tested values of this certificate were found to be in conformance with the specification.

Relevant instrument specifications

Air kerma: 5 % (RQA), 10 % (N-series)

This laboratory is accredited according to ISO/IEC 17025:2017 by the American Association for Laboratory Accreditation (A2LA) and the results shown in this certificate have been determined within the scope of accreditation unless stated otherwise in this certificate.



Certificate number: o60246672i308613-1



Calibration Certificate



Customer
UPSTATE MEDICAL PHYSICS
BLOSSOM DR 1290
14564 VICTOR
US

Laboratory
Unfors RaySafe Inc.
2 Science Road
Glenwood, IL 60425-1586
USA
+1-833-296-9240
customerservice.us@raysafe.com

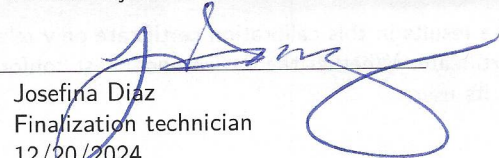
CUSTOMER INSTRUMENT

Product X2 CT
Serial number 308613
Manufacturer RaySafe

CALIBRATION INFORMATION

As found 12/9/2024
As left 12/9/2024
Adjustment done Yes
Tested by Armad Bryant

Approved by


Josefina Diaz
Finalization technician

Certificate date 12/20/2024

CALIBRATION RESULT

AS FOUND: All measured and tested values of this certificate were found to be in conformance with the specification.

AS LEFT: All measured and tested values of this certificate were found to be in conformance with the specification.

Relevant instrument specifications

Air kerma: 5 %

This laboratory is accredited according to ISO/IEC 17025:2017 by the American Association for Laboratory Accreditation (A2LA) and the results shown in this certificate have been determined within the scope of accreditation unless stated otherwise in this certificate.



Calibration Certificate

Customer
UPSTATE MEDICAL PHYSICS
BLOSSOM DR 1290
14564 VICTOR
US

Laboratory
Unfors RaySafe Inc.
2 Science Road
Glenwood, IL 60425-1586
USA
+1-833-296-9240
customerservice.us@raysafe.com

CUSTOMER INSTRUMENT

Product X2 Light
Serial number 300067
Manufacturer RaySafe

CALIBRATION INFORMATION

As found 12/17/2024
As left 12/18/2024
Adjustment done Yes
Tested by Amber Ramos

Approved by


Josefina Diaz
Finalization technician

Certificate date 12/20/2024

CALIBRATION RESULT

AS FOUND: One or more measured and tested values of this certificate are outside of the specifications by a margin less than the expanded measurement uncertainty. Therefore, it is not possible to state non-conformance with specifications for those measurements.

AS LEFT: All measured and tested values of this certificate were found to be in conformance with the specification.

Relevant instrument specifications

Illuminance: 3 %
Luminance: 3 %

